




Associates of Cape Cod, Inc.

Your Endotoxin & Glucan Experts

CELEBRATING OUR 45 YEAR ANNIVERSARY

GEL-CLOT ENDOTOXIN DETECTION TESTING

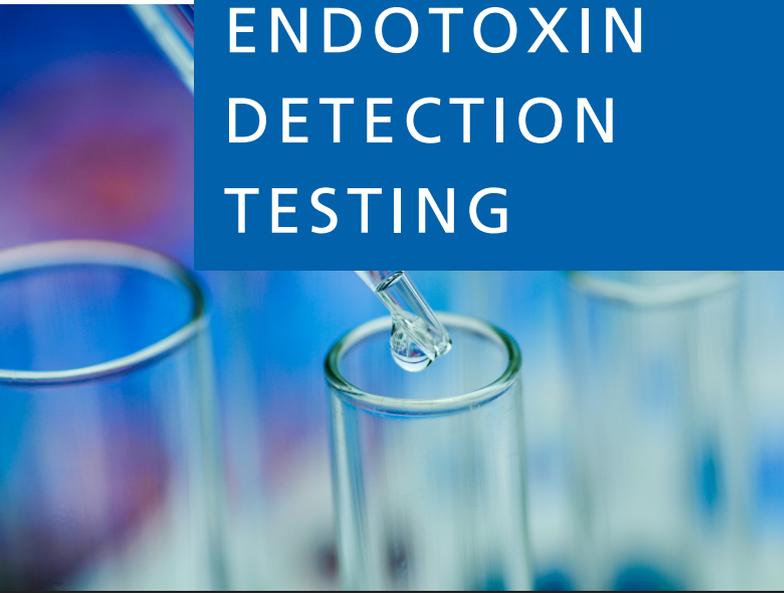

**Our Test, Your Cure...
Ensuring A Healthy World**

Your Endotoxin Experts!

Experts in Endotoxin and Glucan Detection for 45 Years.



THE ORIGINAL GEL-CLOT ASSAY



Pyrotell® Gel-Clot Endotoxin Testing

ACC's Pyrotell® was the first BET reagent licensed by the US FDA. It is easy to use and is available in both economical Multi-Test Vials (MTVs) and convenient Single Test Vials (STVs). Pyrotell® is a robust reagent, producing firm, easily read clots and is resistant to interfering substances. The gel-clot test does not require sophisticated equipment and software and is the simplest BET test to implement.

Sensitivity

Pyrotell® is available in a variety of sensitivities: 0.03 EU/mL; 0.06 EU/mL; 0.125 EU/mL; and 0.25 EU/mL.

Sample to BET Ratio

Reconstituted Pyrotell® reagent is used at a ratio of 1:1 and a volume of 100 µL/test.

Performing the Test

For 2 mL and 5 mL MTV, 100 µL of lysate is mixed with 100 µL of sample in a reaction tube. For STV, 200 µL of sample is added to the vial, which serves as a reaction tube. Test tubes are incubated at 37±1°C for 60 minutes ± 2 minutes. A positive test is indicated if the clot remains solid after the inversion of the test tube.

Reconstitution

Pyrotell® MTV may be reconstituted with BET Reagent Water (LRW), Pyrosol® buffer or Glucashield® buffer, a (1→3)-β-D-Glucan inhibiting buffer, to render the assay endotoxin specific. Pyrotell® STV is reconstituted by the sample being tested.

Stability

Once reconstituted Pyrotell® MTV is stable for 24 hours if stored at 2–8°C. Pyrotell® MTV may be frozen once and will retain activity for as long as 3 months if stored at or below -20°C. STVs are used immediately upon addition of the sample.

Packaging

Pyrotell® is available in 2 mL (approx. 20 tests/vial) or 5 mL (approx. 50 tests/vial) MTV and STV sizes. STV's are sold in 5x10 vial packs. Certificates of Analysis, specific to the Pyrotell® and CSE lot, can be obtained from ACC or online at www.acciusa.com. It is recommended for use with 0.5 µg/vial Control Standard Endotoxin (E0005-1). See page 22 for product vial test quantities.



RAPID ENDOTOXIN DETECTION

Pyrosate® Kit – Rapid Endotoxin Detection

The Pyrosate® kit is an easy-to-use FDA Licensed BET gel-clot test allowing for BET compliant endotoxin testing. The assay does not require special training or laboratory supplies and the step-by-step illustrated instructions allow the user to perform assays within minutes. The Pyrosate® kit provides rapid results and is especially convenient for research, testing water and dialysate.

Sensitivity

The Pyrosate® kit is available in sensitivities of 0.25 EU/mL, 0.125 EU/mL and 0.03 EU/mL. The test may be as short as 30 minutes, depending on the sensitivity.

Performing the Test


The Pyrosate® kit is a rapid gel-clot test that contains a 2λ* endotoxin tube (PPC) matched to the sample (SPL) tube for each sensitivity. This feature is unique to the Pyrosate® assay. The endotoxin tube (PPC) assures that the sample does not interfere with the test, ruling out false negatives. Pyrosate® is formulated to eliminate false positives due to (1→3)-β-D-Glucans. This endotoxin specific reagent does not require additional blocking buffers.

Reconstitution

Pyrosate® is reconstituted directly with the sample by adding 0.5 mL to the sample tube (SPL). After approximately 60 seconds of gentle mixing, 0.25 mL is transferred to the endotoxin tube (PPC). The lot-specific incubation time at 37±1°C is given on the Certificate of Compliance.

Stability

Pyrosate® is stable at room temperature and does not require refrigeration for shipping or storage.

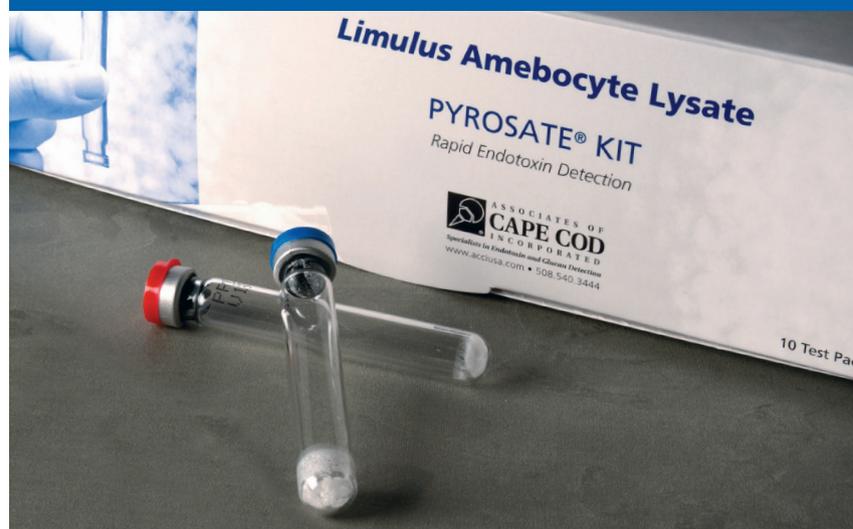

Product Applications

- Hemodialysis
- Water and Water Systems
- Filter Industry
- Research
- Final Product

Product Benefits

- Shorter Assay Time
- Endotoxin Specific
- No Dilutions Required
- No Refrigeration Required
- Matched Positive Product Control

Packaging

The Pyrosate® kit is available in a 10 test kit and a 30 test bulk package for each sensitivity. Each kit contains sample test tubes (SPL) and endotoxin test tubes (Positive Product Control-PPC). A Certificate of Analysis, specific to the Pyrosate® and CSE lot, can be obtained from ACC or online at www.acclusa.com.

*λ (lambda) is the lowest concentration of endotoxin to cause a positive test result under standard conditions.

GEL-CLOT TESTING SUMMARY

Pyrotell®

Multi-Test Vial (MTV), 5 mL/vial
(approx. 50 tests/vial)

#G5003-5	0.03 EU/mL (250 test 5 pack)
#G5003-25	0.03 EU/mL (1250 test 25 pack)
#G5006-5	0.06 EU/mL (250 test 5 pack)
#G5006-25	0.06 EU/mL (1250 test 25 pack)
#G5125-5	0.125 EU/mL (250 test 5 pack)
#G5125-25	0.125 EU/mL (1250 test 25 pack)
#G5250-5	0.25 EU/mL (250 test 5 pack)
#G5250-25	0.25 EU/mL (1250 test 25 pack)

Multi-Test Vial (MTV), 2 mL/vial
(approx. 20 tests/vial)

#G2003-5	0.03 EU/mL (100 test 5 pack)
#G2006-5	0.06 EU/mL (100 test 5 pack)
#G2125-5	0.125 EU/mL (100 test 5 pack)
#G2250-5	0.25 EU/mL (100 test 5 pack)

Single Test Vial (STV), 0.2 mL/vial

#GS003-5	0.03 EU/mL (five 10 vial packs)
#GS006-5	0.06 EU/mL (five 10 vial packs)
#GS125-5	0.125 EU/mL (five 10 vial packs)
#GS250-5	0.25 EU/mL (five 10 vial packs)

Endotoxin Standards

For use in standard preparation and for depyrogenation control vials.

#E0005-1	0.5 µg/vial (1 vial)
#E0005-5	0.5 µg/vial (5 pack)
#E0125-1	125 µg/vial (1 pack)
#E0125-5	125 µg/vial (5 pack)
#EC010-5	10 ng/vial, (5 pack) (for use with Pyrochrome® kits)

Pyrosol® LAL Reconstitution Buffer

#BR051-5	Pyrosol® Buffer with pH indicator (gel-clot only), 5.5 mL/vial 5 pack
#BR051-25	Pyrosol® Buffer with pH indicator (gel-clot only), 5.5 mL/vial 25 pack
#BC051-5	Pyrosol® Buffer without pH indicator 5.5 mL/vial 5 pack
#BC051-25	Pyrosol® Buffer without pH indicator 5.5 mL/vial 25 pack
#BC54-1	Pyrosol® Buffer without pH indicator 5.5 mL/vial 1 pack

Glucashield® (1→3)-β-D-Glucan Inhibiting Buffer

Glucashield® buffer is used to reconstitute LAL and render the reagent insensitive to (1→3)-β-D-Glucan interference by effectively blocking the Factor G pathway of the endotoxin clotting cascade. For use with Pyrotell® Multi-Test Vials, Pyrotell®-T, Pyrochrome® and Chromo-LAL.

#GB051-5	Glucashield® Buffer 5.5 mL/vial (5 pack)
#GB051-25	Glucashield® Buffer 5.5 mL/vial (25 pack)

Pyrosate® Kit

Includes sample test tubes and positive product control test tubes.

#PSD030-10	Pyrosate® 0.03 EU/mL 10-Test Kit
#PSD030-30	Pyrosate® 0.03 EU/mL 30-Test
#PSD125-10	Pyrosate® 0.125 EU/mL 10-Test Kit
#PSD125-30	Pyrosate® 0.125 EU/mL 30-Test
#PSD250-10	Pyrosate® 0.25 EU/mL 10-Test Kit
#PSD250-30	Pyrosate® 0.25 EU/mL 30-Test

Disposable transfer pipettes (PPT50) sold separately.

Accessory Products

LAL Reagent Water (LRW)

LRW is intended for reconstitution of BET reagents, CSE and to dilute samples and standards for BET assays. LRW is not for human or animal injection. LRW contains less than 0.001 EU/mL endotoxin and less than 1.56 pg/mL glucan.

#W0051-10 5.5 mL/bottle, 10 bottles/pack

#W020P 20 mL/bottle, 10 bottles/pack

#WP050C 50 mL/Plastic bottle, 30 bottles/pack

#WP100C 100 mL/Plastic bottle, 30 bottles/pack

#WP500C 500 mL/Plastic bottle, 12 bottles/pack

#WP1000C 1L/Plastic bottle, 12 bottles/pack

Pyrotubes®

#TK100-10 8 x 75 mm borosilicate glass for Pyros Kinetix®, 50 tubes/pack, 10 packs/carton

#TS050-10 10 x 75 mm soda lime glass for gel-clot method, 52 tubes/pack, 10 packs/carton

#TB050-5 10 x 75 mm borosilicate glass for turbidimetric method, 52 tubes/pack, 5 packs/carton

#TB240-5 12 x 75 mm borosilicate glass (for dilutions only), 42 tubes/pack, 5 packs/carton

#TB013-5 13 x 100 mm borosilicate glass, 18 tubes/pack, 5 packs

#TB16C 16 x 90 mm depyrogenation tubes with Aluminum caps, 65/pack


Pipette Tips

#PPT25 250 µL tips, 96 tips/box, 10 boxes/pack

#PPT10 1000 µL tips, 96 tips/box, 8 boxes/pack


#PPT50 Disposable Transfer Pipettes 50/pack
(for use with Pyrosate® kits)

Availability of ancillary products varies depending upon the local office.

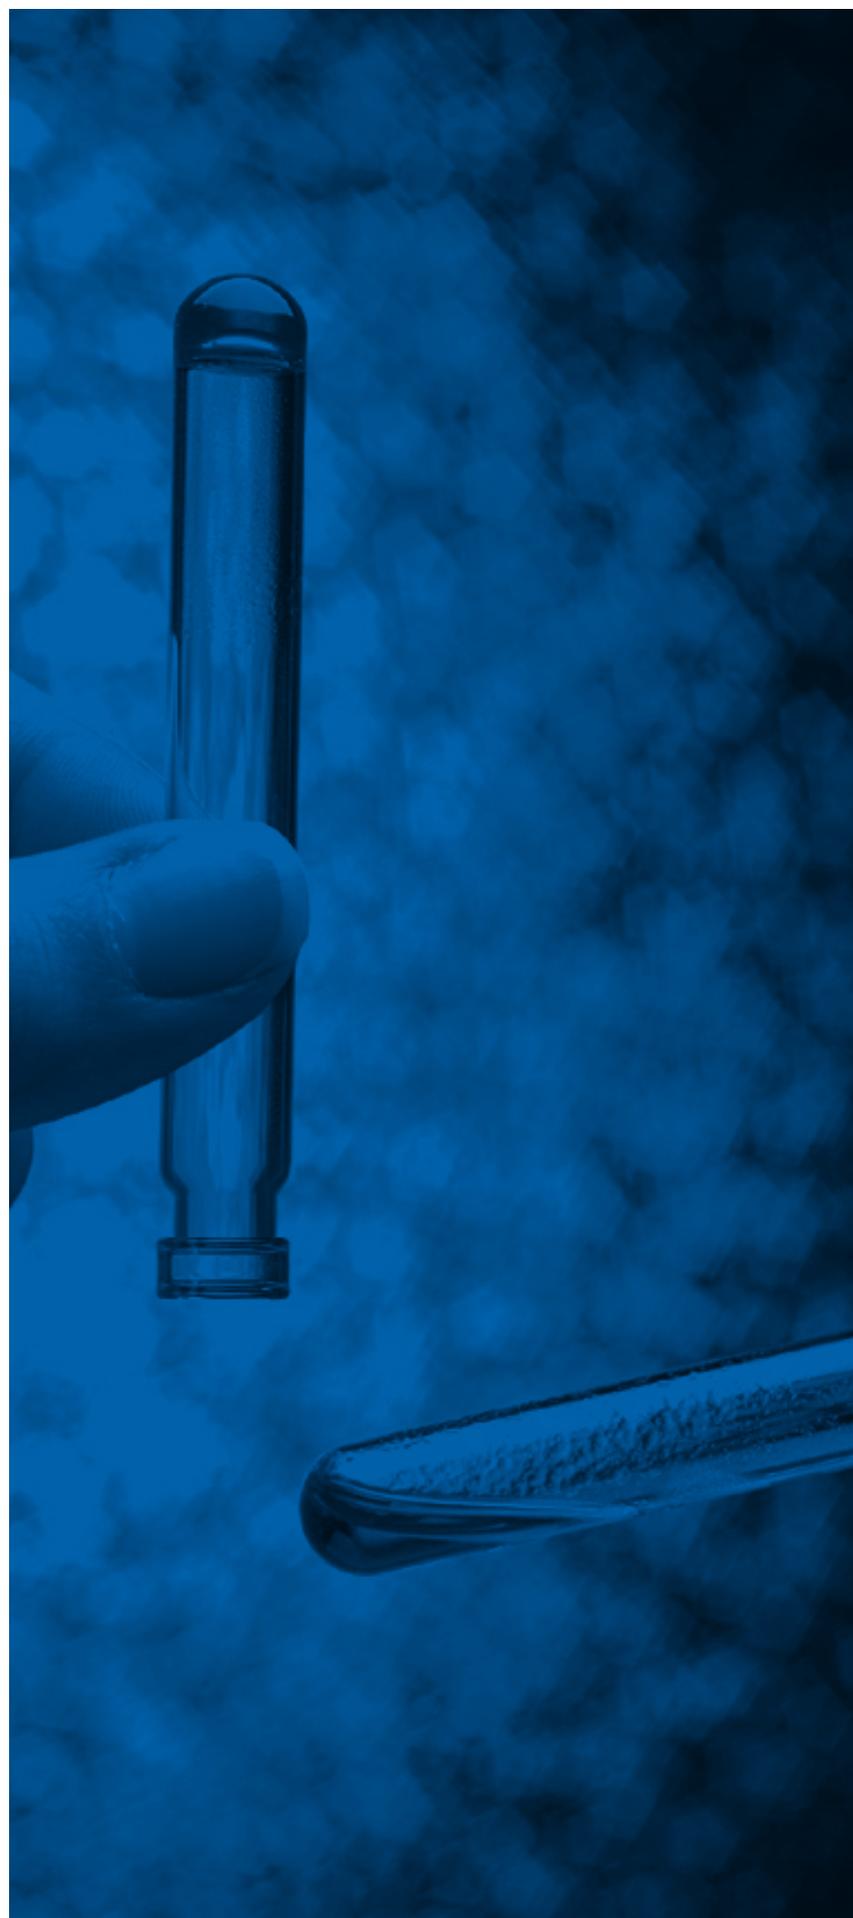

PYROSATE[®]

RAPID ENDOTOXIN DETECTION KIT

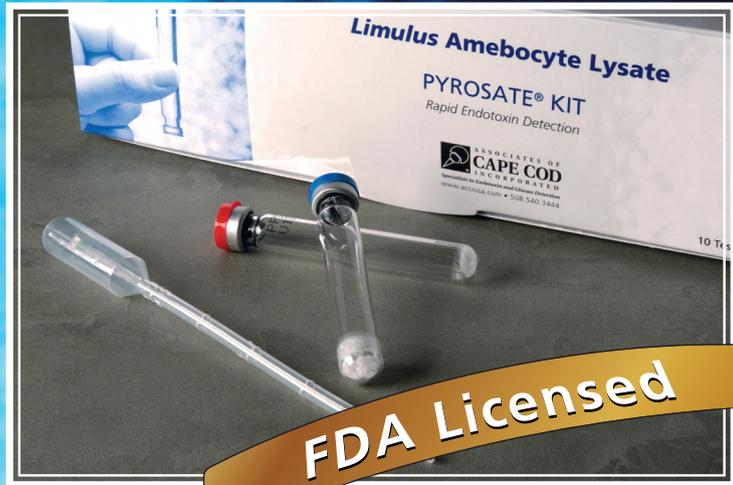

FDA Licensed

New Sensitivities Of
0.03, 0.125 and 0.25 EU/mL

Final Product Release

Easy-To-Use Method

Rapid Test Results

Bacterial Endotoxin Testing
USP Chapter <85> Compliant



Associates of Cape Cod, Incorporated

124 Bernard E. Saint Jean Dr., East Falmouth, MA 02536 USA
888.395.2221 • INFO@ACCIUSA.COM • WWW.ACCIUSA.COM

ORDERING INFO AND SALES OFFICES



Ordering Information

Customer service representatives are available to assist you with orders, pricing requests and Certificates of Analysis.

Method of Payment For United States

- Check (in US dollars) made payable to Associates of Cape Cod, Inc.
- Wire Transfer (contact Accounts Receivable for routing information)
- Credit Card (AMEX®, VISA®, MasterCard®)
If payment is to be made by credit card, the following information is required: Type of Credit Card, Card Number, Credit Card Security Code, Expiration Date of Card, and Name (as it appears on the card).

Additional Information

ACC reserves the right to institute, modify or discontinue credit limits provided to customers at any time for any or no reason.

The use of credit cards for payment may incur a fee, please see our website for ACC's policy on credit card usage at www.acciusa.com/pdfs/acctc.pdf

Outside the U.S.

Please contact your local office for information regarding method of payment. For a list of your country specific distributors please visit www.acciusa.com.

Product listings, information and fill sizes are subject to change at any time without prior notice.

Corporate Headquarters

Associates of Cape Cod, Inc.

124 Bernard E. Saint Jean Drive
East Falmouth, MA 02536-4445 USA
Tel: (800) LAL-TEST (525-8378) or (508) 540-3444
Fax: (508) 540-8680
www.acciusa.com
Customer Service: custservice@acciusa.com
Technical Service: techservice@acciusa.com
Contract Test Service: testservice@acciusa.com

United Kingdom

Associates of Cape Cod Int'l., Inc.
Deacon Park, Moorgate Road
Knowsley, Merseyside, L33 7RX, United Kingdom
Tel: (44) 151-547-7444
Fax: (44) 151-547-7400
E-mail: info@acciuk.co.uk
www.acciuk.co.uk
UK Customer Service: customerservices@acciuk.co.uk
Company Registration Number: BR002906

Europe

Associates of Cape Cod Europe GmbH
Opelstrasse 14
D-64546 Mörfelden-Walldorf, Germany
Tel: (49) 61 05-96 10 0
Fax: (49) 61 05-96 10 15
E-mail: service@acciusa.de
www.acciusa.de

All Products and Services listed herein are offered exclusively under Associates of Cape Cod, Inc.'s Terms and Conditions of Sale which can be found at www.acciusa.com/pdfs/acctc.pdf



ASSOCIATES OF
CAPE COD
INCORPORATED

Specialists in Endotoxin and Glucan Detection

Corporate Headquarters

Associates of Cape Cod, Inc.

124 Bernard E. Saint Jean Drive
East Falmouth, MA 02536-4445 USA
Tel: (800) LAL-TEST (525-8378) or
(508) 540-3444

Fax: (508) 540-8680

www.acciusa.com

Customer Service:

custservice@acciusa.com

Technical Service:

techservice@acciusa.com

Contract Test Service:

testservice@acciusa.com

United Kingdom

Associates of Cape Cod Int'l., Inc.

Deacon Park, Moorgate Road
Knowsley, Liverpool, L33 7RX
United Kingdom

Tel: (44) 151-547-7444

Fax: (44) 151-547-7400

E-mail: info@acciuk.co.uk

www.acciuk.co.uk

UK Customer Support:

customerservices@acciuk.co.uk

Company Registration Number:

BR002906

Europe

Associates of Cape Cod Europe GmbH

Opelstrasse 14
D-64546 Mörfelden-Walldorf
Germany

Tel: (49) 61 05-96 10 0

Fax: (49) 61 05-96 10 15

E-mail: service@acciusa.de

www.acciusa.de